

Improved Sensitivity for the Detection of Per- and Polyfluorinated Alkyl Substances (PFAS) in Environmental Water Samples Using a Direct Injection Approach on Xevo™ TQ Absolute



Xevo™ TQ ABSOLUTE

歡迎掃描詳看文章內容

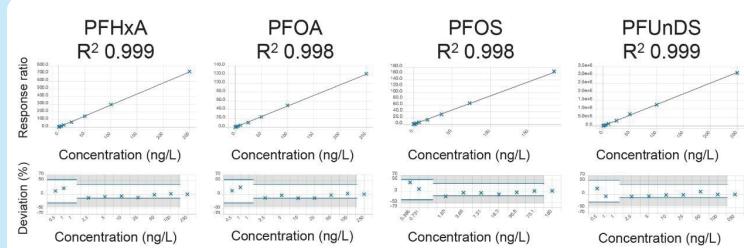


Figure 1. Calibration data of four PFAS compounds demonstrating calibration curve linearity and calibration deviation.

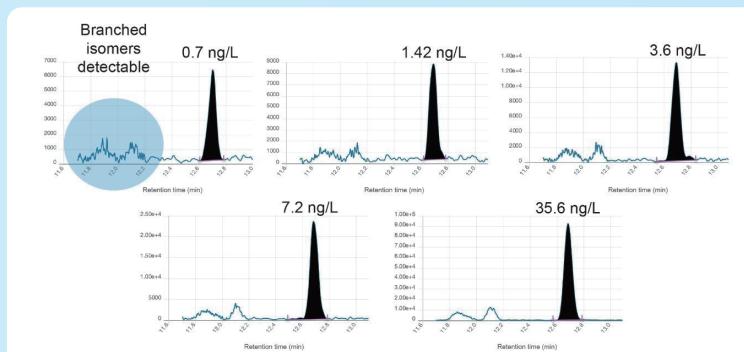


Figure 2. PFOS in wastewater influent at various spiked concentrations.